<Note>
1) Detail information about foundation is available upon request, if any.

2) The primary piping of cooling water shoul be made using flexible piping such as a rubber hose. And also, the inlet wiring of power source should made using flexible cable such as a rubber sheath cord.

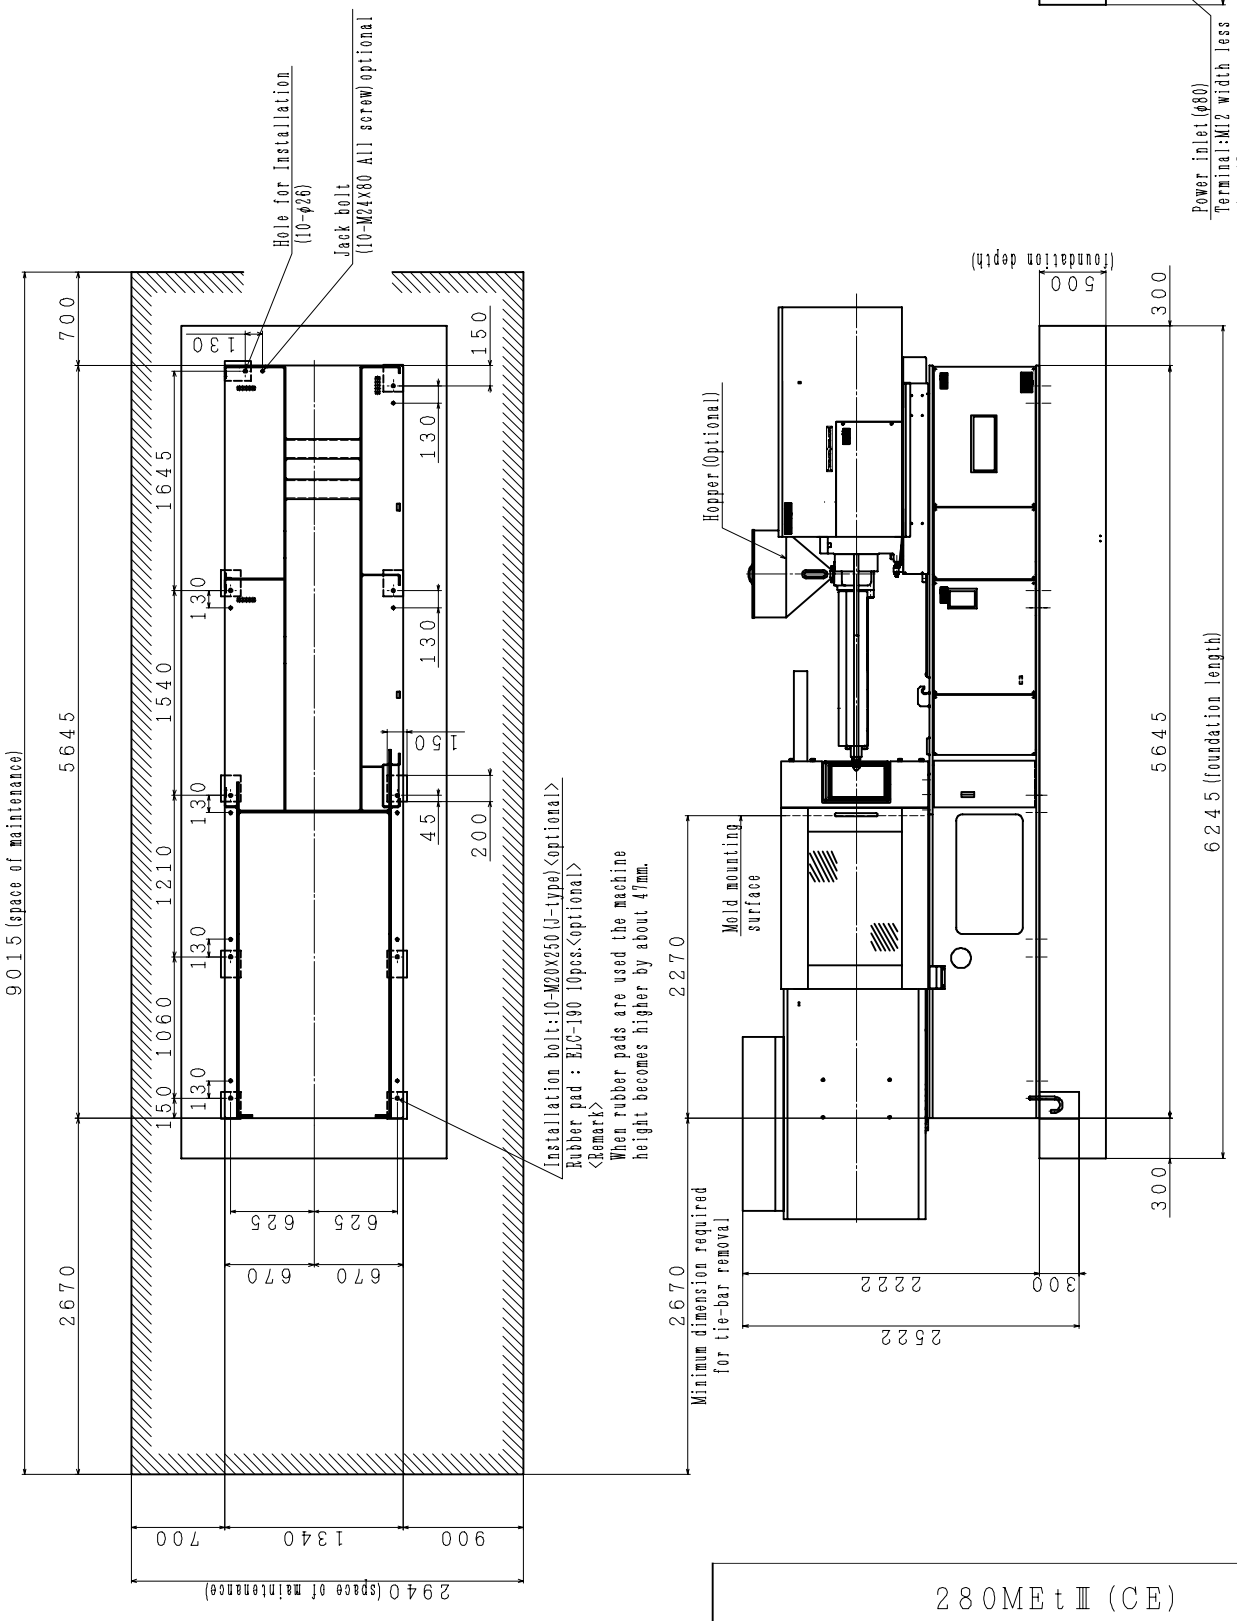

280MEtⅢ(CE)	
9−2 FOUNDATION DRAWING	

10−900